



Xenon light source



Microfluidic Reagent Rotor


7 minutes

Sample-to-answer in
3 simple steps and
approximately 7 minutes



MNCHIP - Clinical Chemistry +

Chemistry Analyzer Celercare® cV5

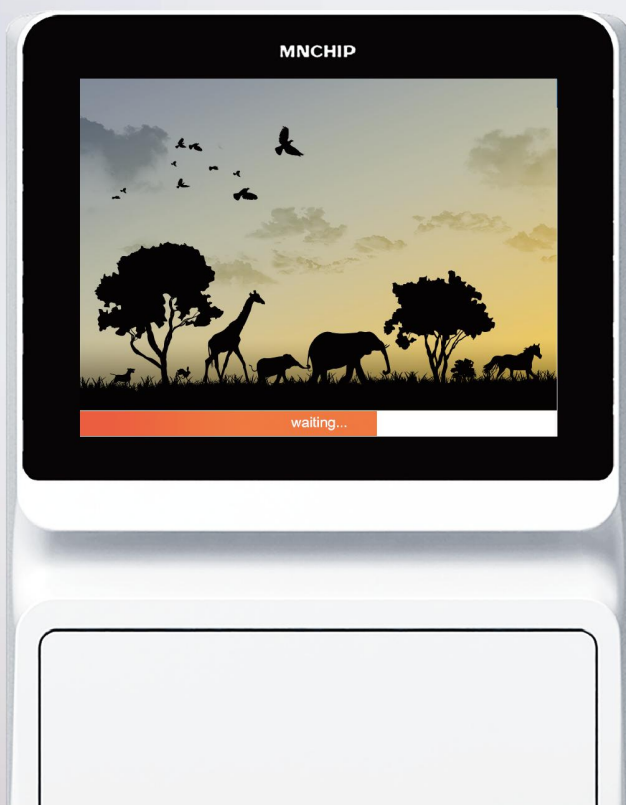

MNCHIP

The diagram illustrates the layout of a 96-well microplate. It features a circular arrangement of wells. Labels with leader lines point to specific wells: 'Reaction Cuvette' points to a well in the top right quadrant; 'Diluent' points to a well in the middle left quadrant; and 'Sample Port' points to a well in the bottom right quadrant. A red 'X' is also visible in the bottom center area.

MNCHIP All rights reserved.